CS Prone Plus Face Cushion

*Suitable for patients 8 years+

Product code: CSM2512

Ensure the eyebrows are visible to avoid direct pressure to the eyes.
Use with CSM2565 (CSM2567 & CSM2565-1) and other compatible head support systems

⚠ Only to be used by trained clinicians.



1 With patient supine, disconnect ET tubing

2 Place cushion onto patient's face*



3 Place helmet (CSM2565-1) over cushion



4 Turn patient to prone position

5 Re-connect ET Tubing

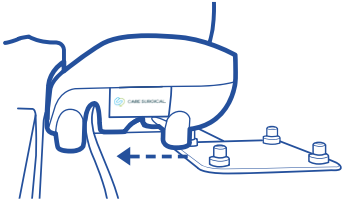

6 Lift helmet & locate onto mirror's cogs

7 Check face is correctly positioned in cushion*

8 Adjust cogs to obtain neutral neck line

250kg Maximum Patient Weight

MD

LATEX

NON STERILE

UK: Care Surgical Ltd
Unit 6 Ringtail Road,
Burscough,
L40 8JY
Tel: 01704 336671

USA: Care Surgical LLC
43 Broad Street
Suite B106, Hudson,
MA 01749, USA
Tel: 866-243-4107

www.care-surgical.com

EU REP

Care Surgical Supplies Limited, Office 2, 12a Lower Main Street, Lucan Co. Dublin, K78 X5P8 Ireland

⚠ **DO NOT REUSE**! if reused injury to patient could occur due to issues with infection control and deterioration of the product.

⚠ **SAFE DISPOSAL**: customers should adhere to any local laws and regulations to the safe disposal of medical devices.

⚠ **DO NOT USE** products that appear to be damaged or worn. In an event of product damage or patient injury, please contact Care Surgical.

5 060624 120008

Ref: CSM2512 - IFU (Rev.15) 04/2025

The Forehead & Cheeks

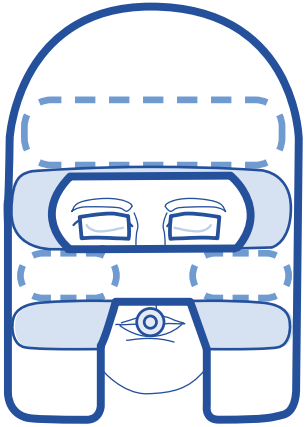

See the instructional video at www.care-surgical.com

Possible problems

+ Pressure ulcers
+ Facial edema

Possible causes

+ Inadequate blood supply due to prolonged excessive pressure
+ Shear, affecting the blood flow to the forehead or cheeks
+ Friction injury due to a period of continuous movement
+ Patient incorrectly positioned in the face support
+ High risk patient (includes the elderly, diabetics, smokers and those taking certain medications, eg steroids)

Reduce the risk

+ Ensure the patient's face is supported on the bony part of their cheeks, not the soft tissue
+ Ensure the patient's eyebrows are clearly visible
+ The face support must not encroach into the periorbital area above or below the eye
+ Recheck the head support after turning the patient and at least every 30 minutes throughout the procedure
+ It may be necessary to lift and replace the patient's face during long procedures or if there has been movement

UK: Care Surgical Ltd
Unit 6 Ringtail Road,
Burscough,
L40 8JY
Tel: 01704 336671

USA: Care Surgical LLC
43 Broad Street
Suite B106, Hudson,
MA 01749, USA
Tel: 866-243-4107

www.care-surgical.com

EU REP
Care Surgical Supplies Limited, Office 2, 12a Lower Main Street,
Lucan Co. Dublin, K78 X5P8 Ireland

250kg Maximum Patient Weight

MD

UK CA

LATEX

NON STERILE

5 060624 120008

Ref: CSM2512 - IFU (Rev.15) 04/2025